

Care and Maintenance of Your Ride Cushion

Cleaning the outer cover


- Remove your Ride Forward Cushion from the wheelchair.
- Remove the outer cover from the Cushion. Zip cover closed.
- Machine or hand wash in warm water (regular detergent/no bleach). Hang dry.

Cleaning the Cushion

- The moisture resistant inner cover is designed to protect the foam materials of the cushion and should not be removed. If soiled, simply wipe clean with a damp cloth.
- Once dry, insert the cushion into the cover. Ensure that the cover is placed correctly front to back.
- Place the Cushion on your wheelchair so that the rear of the cushion, identifiable by the content tags, is flush with the back of the sling or solid seat.

WARNING:

- The Ride Forward materials work optimally at room temperature. Always allow the Ride Forward cushion to come to room temperature before use. Sitting on excessively warm or cold surfaces can cause skin damage.

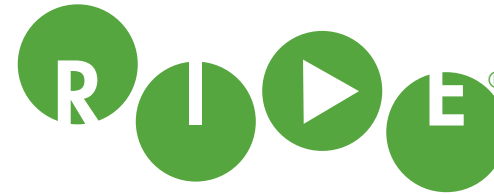

Ride Forward™ Cushion Owner's Handbook

► Warranty Policy Installation and Use Instructions Care and Maintenance

Warranty Policy

Your Ride Forward Cushion has been carefully constructed to meet your wheelchair seating needs. This Limited Warranty is effective for 24 months from the date of delivery to the original purchaser. If any defect in material or workmanship is found, Ride Designs® will repair or replace the component, at our discretion. This limited warranty does not cover daily wear and tear or damage that is a result of mishandling, misuse, neglect, or not following the care and maintenance instructions.

Your cushion cover is under warranty for 90 days. The warranty includes damage due to workmanship, material defects or errors caused by the manufacturer. This warranty does not apply to cigarette burns, damage to the cover by sharp objects that may cause tears, or damage as a result of not following the washing instructions.

Claims and repairs should be processed through your nearest authorized Ride Designs rehab technology supplier. A copy of the Bill of Sale issued to the purchaser of the product may be required prior to processing a warranty claim.

Maximum client weight capacity is 250 pounds.

► **Ride Designs®**
a branch of Aspen Seating, LLC
4211-G South Natches Court
Sheridan, Colorado 80110

toll-free: 866.781.1633
phone: 303.781.1633
www.ridedesigns.com

Ride Forward Cushion General Product Safety

Safe application of this product depends upon your good judgment and common sense, as well as that of your provider, caregiver, and/or healthcare professional and your attentiveness in following the warnings, cautions, notes, and instructions in this manual.

NOTE: Denotes important things to remember when using this product.

WARNING: Indicates a potentially dangerous situation which, if not heeded, could result in serious injury.

CAUTION: Failure to heed cautions may result in damage to your product.

NOTE: Ride Designs is not liable for damage to property or personal injury arising out of unsafe use of this product. Ride Designs is also not liable for any property damage or personal injury arising out of the failure of any person and/or user to follow the instructions or recommendations set forth in 1) this manual, or 2) any other instructions or recommendations contained in related literature issued by Ride Designs, or 3) contained on the product itself.

NOTE: We have compiled this manual from the latest specifications and product information available at the time of publication. We reserve the right to make changes as they become necessary. Any changes to our products may cause slight variations between the illustrations and explanations in this manual and the product you have purchased.

WARNING: All Ride Designs cushions are designed to help reduce the incidence of pressure sores. However, no cushion can completely eliminate sitting pressure or prevent pressure sores. Ride Designs cushions are not a substitute for good skin care including proper diet, cleanliness, and regular pressure relief techniques.

Installation and Use Instructions


It is recommended that a supplier or therapist certified by Ride Designs conducts the initial fitting of your cushion. Your Ride Forward Cushion, in conjunction with its unique cover, is designed to comfortably stabilize your posture and help reduce your risk for skin breakdown.

Preparing the wheelchair for your Ride Forward Cushion

Your Ride Forward Cushion is designed to work on both sling style or solid seat inserts.

NOTE: If your sling seat presents with a gap between the Cushion bottom and sling upholstery, the upholstery must be tightened or replaced.

CAUTION: The Ride Forward Cushion must not extend more than 1" beyond the front of your wheelchair's sling or solid seat.

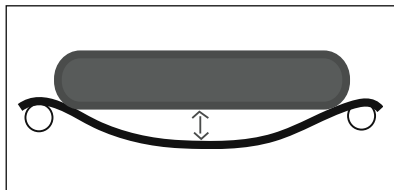

Install and fit your Ride Forward Cushion

WARNING: Installing a cushion on a wheelchair may affect the center of gravity of the wheelchair and may cause the wheelchair to tip backwards, potentially resulting in injury. Always assess for the potential need for anti-tippers or amputee axle adapter brackets to be added to your wheelchair to help increase stability.

WARNING: Improper placement or securement of the Ride Forward Cushion to your wheelchair may result in serious injury. Your wheelchair must have complementary hook fastener on the sling or solid seat to properly secure the Cushion.

WARNING: Failure to accurately assess and fit the Ride Forward Cushion may result in serious injury to the user.

1. Place the cushion on the wheelchair so that the rear of the cushion, identifiable by the content tags, is flush with the back of the sling or solid seat. Ensure that the loop fastener on the bottom of your Forward cover engages with hook fastener on the sling or solid seat of your wheelchair.

2. Transfer gently onto the cushion. Lean forward at the trunk and scoot your bottom to the back of the cushion. Ensure that your trochanters (hip bones) rest within the relief on the sides of the cushion and that your gluteal muscles are supported on the back corners of the cushion.

3. Adjust your footrest height so that your legs rest comfortably on the front of the cushion. Accurate footrest height is imperative for optimal cushion performance.

WARNING: If you are unable to achieve sufficient skin protection, postural control, and/or are unable to tolerate sitting on the cushion for any reason, then the Ride Forward Cushion is not an appropriate cushion choice and a Ride Custom Cushion should be considered. Contact Ride Designs or your certified Ride Designs supplier for more information about the Ride Custom Cushion.

Initial wearing schedule

Prior to prolonged sitting, it is advisable to sit in your Cushion for short periods of time. Make sure to visually check any area that contacts the Cushion after each period of use. Any reddened area should fade within 10-30 minutes. Contact your doctor or therapist if the redness persists for greater than 30 minutes. As long as skin inspections do not show red areas persisting more than 30 minutes, extend the length of sitting time gradually (½ to 1 hour each day). Continue skin checks after each increased sitting time. Two to four hour periods are the general recommended maximum time in the sitting position. Skin checks should be made no less than daily, even after skin tolerance is established. Continue to perform routine intermittent pressure relief techniques (either manual lifts or weight shifts using power tilt) as advised by your healthcare professional.

WARNING: If any redness associated with the use of the Forward cushion persists for greater than 30 minutes, then cease sitting on the cushion and contact your therapist or doctor immediately.

Follow-up

It is recommended to have your seated posture and skin integrity checked by your healthcare professional at least annually, or whenever you experience a change in your weight, posture, or general condition that could impact your ability to sit safely, comfortably, and functionally.